

Validation report:

***Alexandromys oeconomus* qPCR detection kit**

with eDNA qPCR hot start mix

#SYL109

Document date: 15 November 2022

For general laboratory and research use only

Index

1. Validation report <i>Alexandromys oeconomus</i> detection kit	4
1.1 In silico validation.....	4
1.2 Experimental validation	5
1.2.1 Optimal annealing temperature primers.....	5
1.2.2 detection limit, fluorescence output signal and efficiency.....	5
1.2.3 Influence of inhibiting factors present in environmental samples and repeatability.....	7
1.2.4 Detection conformation of <i>Alexandromys oeconomus</i> in environmental samples	8
1.2.5 Sequence conformation of specificity.....	8
1.3 Summary of validation	9
1.3.1 Robustness	9
1.3.2 Detection limit.....	9
1.3.4 Efficiency	9
1.3.5 Repeatability	9
1.3.6 Correctness	9

1. Validation report *Alexandromys oeconomus* detection kit

1.1 In silico validation

Table 1: Forward primer *in silico* validation

Length	20
GC %	60
Stability	4.2
T_M (°C)	66
Target region	CytB (mtDNA)
Dimer	No
Run	No
Database hit	<i>Alexandromys oeconomus</i>

Table 2: Reverse primer *in silico* validation

Length (bp)	23
GC %	39
Stability	1.0
T_M (°C)	64
Target region	CytB (mtDNA)
Dimer	No
Run	No
Database hit	<i>Alexandromys oeconomus</i>

Table 3: Probe *in silico* validation

Length	32
GC %	37
T_M (°C)	70
Target region	CytB (mtDNA)
Dimer	No
Run	No
Fluorescence label	FAM

Table 4: Combined primers and probe *in silico* validation

PCR product size (bp)	91
Combined dimer formation	No
<i>In silico</i> PCR on Genbank	<i>Alexandromys oeconomus</i>
Date of <i>In silico</i> PCR	November 2022

1.2 Experimental validation

All validation experiments were performed with the Sylphium qPCR mix and performed on Applied biosystems 7300 qPCR machines and Biometra gradient PCR machines.

1.2.1 Optimal annealing temperature primers

The annealing temperature has a strong influence on the performance, robustness and specificity of the primer set. To determine the optimal annealing temperature, a temperature gradient PCR between 50°C and 67.4°C was performed in eight steps.

Results:

The expected product was formed at all tested temperatures (50.8°C to 67.4°C). (See table 7)

Table. 8: Temperature gradient PCR on genomic DNA of *Alexandromys oeconomicus*.

Annealing temp.	50.8°C	52.3°C	56.0°C	58.°C	60.0°C	62.0°C	65.0°C	67.4°C
Expected fragment	Strong	Strong	Strong	Strong	Strong	Strong	Strong	Strong
Primer dimer	No	No	No	No	No	No	No	No
Additional fragments	No	No	No	No	No	No	No	No

1.2.2 detection limit, fluorescence output signal and efficiency

Standard solutions with 10^5 , 10^4 , 10^3 , 10^2 , 10, 1 and 0 target copies per 5 µl were analyzed to determine the detection limit at optimal primer/probe concentrations. Fluorescent output signals were compared with the background to have at least a 100 fold increase in fluorescence signal. Reaction condition were adjusted if the fluorescence signal was too low in contrast to the background noise. Based on the slope of the standard curve the efficiency of the primer/probe set was determined. The efficiency should be between 90% and 110%. Limits of quantification and detection were determined on basis of this efficiency limitations.

Results:

The detection limits (low and high) for qualitative detection was determined between 1 and $>10^5$ target copies per reaction. The detection limits (low and high) for quantitative detection was determined between 10 and $>10^5$ target copies per reaction. The fluorescence output signal was at least 100 (8 for positive sample, 0,01 for a negative sample) times stronger than the background signal. (fig. 1). The efficiency of the test was above 90%. Which means that the efficiency of the primer/probe mixture can be regarded optimal (Fig. 2, table 7).

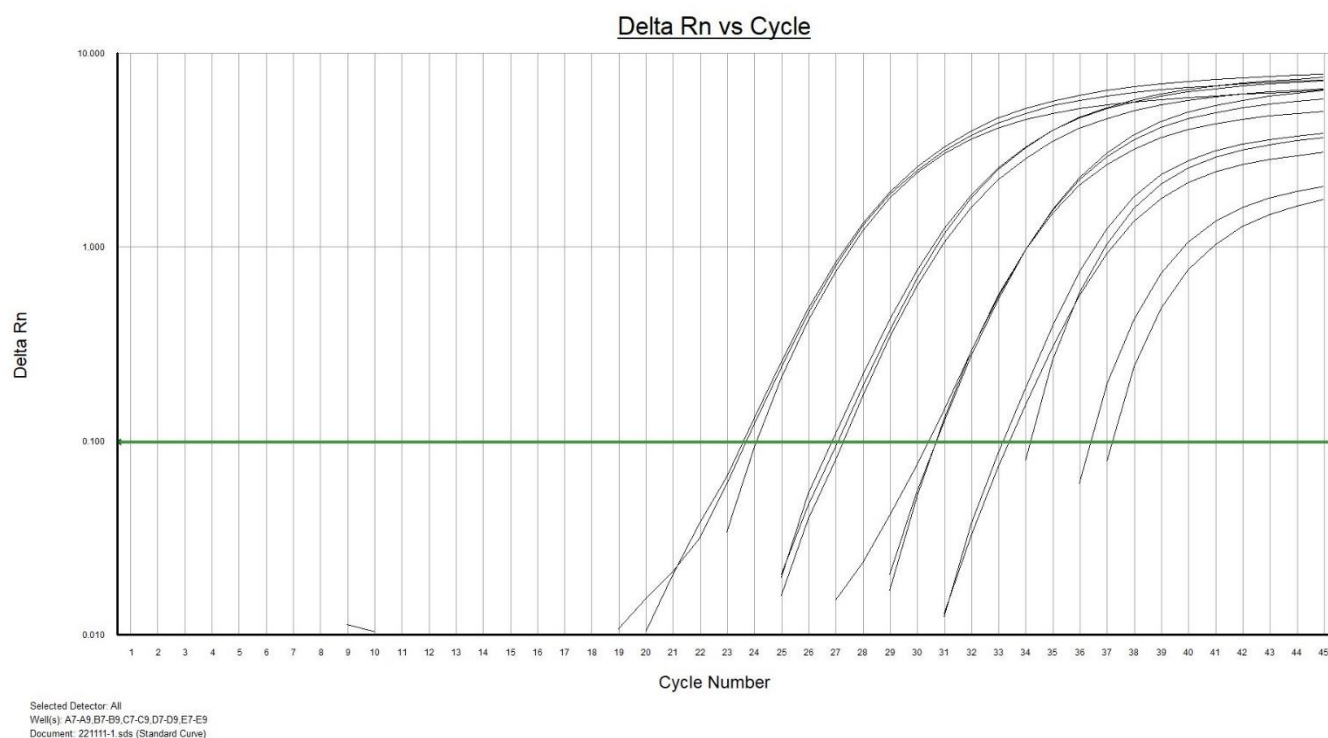


Figure. 1: Obtained fluorescent signal at optimal primer/probe concentration at a annealing temperature of 60°C.

Table 6: CT values obtained at optimal primer/probe concentration.

target DNA copy	Target detected	CT value	Standard deviation
0	No	n.a.	n.a.
1	2 out of 3	n.a.	n.a.
10	Yes	33.7	0.6
10 ²	Yes	30.5	0.2
10 ³	Yes	27.0	0.2
10 ⁴	Yes	23.7	0.3

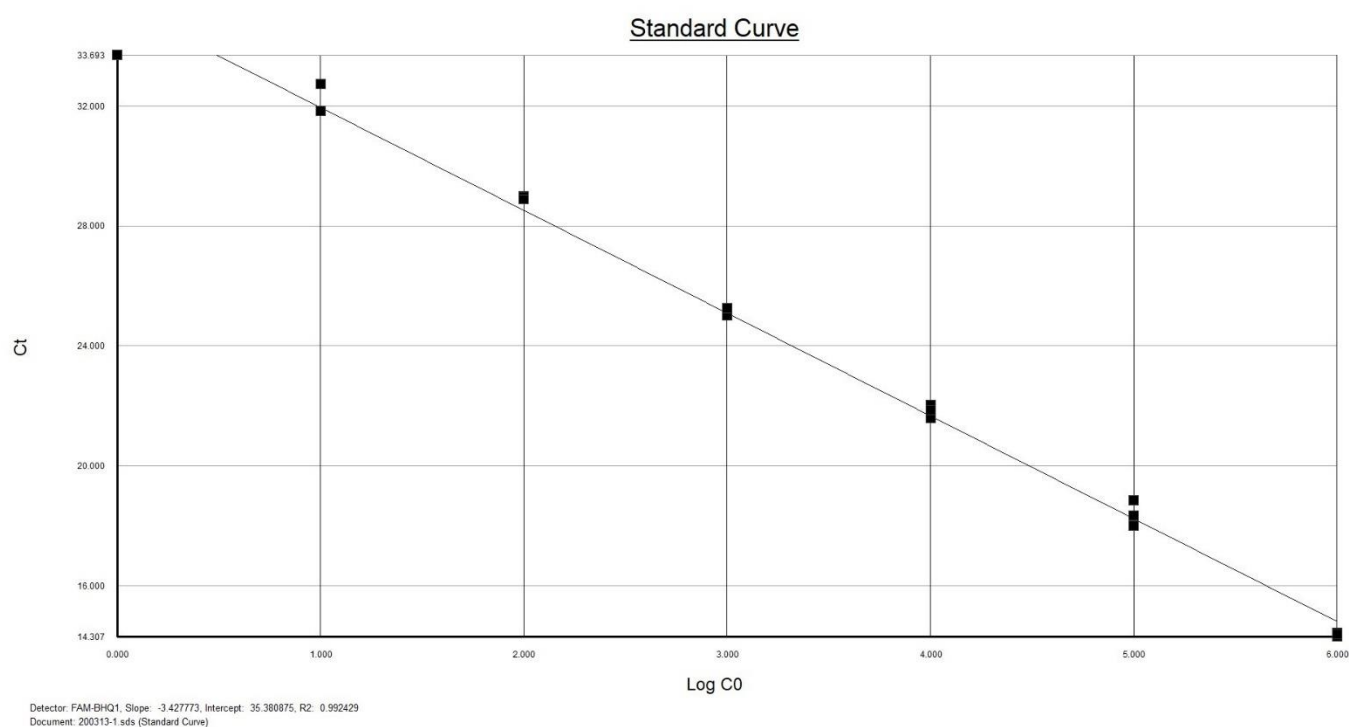


Fig. 2: Standard curve of SYL109 based on 10, 10², 10³, 10⁴ and 10⁵ DNA target copies

Table 7: Values obtained from the standard curve

Slope	-3.43
Efficiency	95.7%
R ²	0.992

1.2.3 Influence of inhibiting factors present in environmental samples and repeatability

Performance of the assay was tested on the influence of inhibiting factors present in three different kinds of environmental water samples (sandy, clayey or peaty bottoms) in three fold spiked with 1000 target DNA copies. The ΔC_T between spiked samples and spike only was determined and should be less than 2. Standard deviations and the standard error of mean were calculated to determine robustness, repeatability and measurement uncertainty.

Results:

No fluorescent output signal was detected in the environmental samples without added target organism DNA (spike). Spiked samples and the spike only analyses gave in all replicates a positive signal. (see table 8). In all cases the ΔC_T was less than 2.

Table 8: CT values obtained with target organisms free environmental samples spiked with 1000 target copies.

Sample	CT value	Standard deviation	Δ CT
Sandy	-	-	-
Clayey	-	-	-
Peaty	-	-	-
Sandy + spike	28,4	0.2	0.1
Clayey + spike	28.7	0.2	0.4
Peaty + spike	28.7	0.3	0.4
Spike only	28.3	0.0	-

1.2.4 Detection conformation of *Alexandromys oeconomicus* in environmental samples

The amount of eDNA that a target organism leaves in the environment depends on the type of target organism, environmental factors and season (CEN / TC230-water analysis, proposal documented in N 1229). To determine the minimal filtration volume, samples were taken at locations where *Alexandromys oeconomicus* may occur, during the optimal seasons (spring, summer and autumn). Samples were taken with SYL009 - Environmental Sampling Kit and eDNA was isolated with SYL002 - Environmental DNA Isolation Kit.

Results:

The kit SYL109 - *Alexandromys oeconomicus* detection kit was able to detect *Alexandromys oeconomicus* in environmental samples from different location in the Netherlands. Positive water samples gave 1 to 100 molecules *Alexandromys oeconomicus* DNA when 750 ml water was filtrated. A positive dropping sample gave $10^3 - 10^6$ molecules.

1.2.5 Sequence conformation of specificity.

PCR products obtained from the environmental samples where the presence of *Alexandromys oeconomicus* was suspected were sequenced for conformation of identity of the formed product. If any product was formed with target organism free environmental samples, than these products were also be sequenced.

Results:

Target organism free environmental samples did not give any PCR product. PCR products obtained from environmental samples were sequenced in triplo via the Sanger sequencing method. The obtained sequences were identical to each other and Blast[®] hits confirmed identity of the target organism.

1.3 Summary of validation

1.3.1 Robustness

“Influence of temperature variations and inhibiting factors present in environmental samples on the performance and specificity of the primer set”

- Primers specific at temperature range: 50.8°C to 67.4°C C (section 1.2.1, table 5)
- Influence of chemical and biological factors present in environmental samples on the performance of the test were not found. (section 1.2.3, table 8)
- Fluorescent output signals of positive samples is at least 100 fold stronger than the background

1.3.2 Detection limit

“Limits (lower and upper limit) within which the analysis can be reliably applied”

- Limit of detection (LOD) for this kit was determined on 1 copy per reaction. Limit of quantification (LOQ) was also determined on 10 copies per reaction. (section 1.2.2, table 6)
- The theoretical minimal sampling volume for *Alexandromys oeconomicus* is 750 ml. (section 1.2.4)

1.3.4 Efficiency

“The comparison of what is actually produced with what can be achieved with the same consumption of resources”

The efficiency of the primer set is 95.7 %, this means that the primer/probe mixture can be regarded as optimal. (section 1.2.2, table 7)

1.3.5 Repeatability

“The degree of similarity between the results of measurements of the same measured quantity that were performed under different measurement conditions”

There was no difference ($\Delta CT < 2$) between different kinds of environmental water samples (sandy, clayey or peaty bottoms) spiked with 1000 target DNA copies. (section 1.2.3, table 8)

1.3.6 Correctness

“The ability of the method to do what it 'says' to do”

- The test was able to detect *Alexandromys oeconomicus* DNA in environmental samples from locations where the presence of *Alexandromys oeconomicus* was suspected. (section 1.2.5)
- The method did not give any other combined BLAST hit than the target organism *Alexandromys oeconomicus*
- The method was able to detect all spiked target DNA in target organism free environmental samples (section 1.2.3, table 8)
- The method did not give any signal in target organism free environmental samples (section 1.2.3, table 8)