

Validation report:

***Thaumetopoea processionea* qPCR detection kit**

with eDNA qPCR hot start mix



#SYL110

Document date: 18 May 2022

For general laboratory and research use only.
Cover photo: Sarefo (CC BY-SA 3.0)

Index

1. Validation report <i>Thaumetopoea processionea</i> detection kit	4
1.1 In silico validation.....	4
1.2 Experimental validation	5
1.2.1 Gradient PCR	5
1.2.2 detection limit and fluorescence output signal	5
1.2.3 Efficiency	6
1.2.4 Influence of inhibiting factors present in environmental samples and repeatability.....	7
1.2.5 Detection conformation in environmental samples.....	8
1.2.6 Sequence conformation of specificity.....	9
1.3 Summary of validation	10
1.3.1 Robustness	10
1.3.2 Detection limit.....	10
1.3.4 Efficiency	10
1.3.5 Repeatability	10
1.3.6 Correctness	10

1. Validation report *Thaumetopoea processionea* detection kit

1.1 In silico validation

Table 4: Forward primer *in silico* validation

Length	21
GC %	52
Stability	1.3
T _M (°C)	65
Target region	COI (mtDNA)
Dimer	No
Run	No
Database hit	<i>Thaumetopoea processionea</i>

Table 5: Reverse primer *in silico* validation

Length (bp)	22
GC %	50
Stability	2.2
T _M (°C)	63
Target region	COI (mtDNA)
Dimer	No
Run	No
Database hit	<i>Thaumetopoea processionea</i>

Table 6: Probe *in silico* validation

Length	41
GC %	33
T _M (°C)	75
Target region	COI (mtDNA)
Dimer	No
Run	No
Fluorescence label	FAM

Table 7: Combined primers and probe *in silico* validation

PCR product size (bp)	210
Combined dimer formation	No
<i>In silico</i> PCR on Genbank	<i>Thaumetopoea processionea</i>
Date of <i>In silico</i> PCR	May 2022

1.2 Experimental validation

All validation experiments were performed with the Sylphium qPCR mix and performed on Applied biosystems 7300 qPCR machines and Biometra gradient PCR machines.

1.2.1 Gradient PCR

Influence of the annealing temperature on the performance and specificity of the primer set was tested with a temperature gradient between 50.0°C to 72.0°C in eight steps. Optimal temperature and the temperature range in which the test can perform was determined.

Results:

The expected product was formed between 50.0°C and 67.6°C. No nonspecific additional fragments were formed. No primer dimer were formed at any tested temperature. The optimal annealing temperature was between 50.0°C and 67.6°C (table 8).

Table. 8: Temperature gradient PCR on genomic DNA of *Thaumetopoea processionea*.

Annealing temp.	50.0°C	52.1°C	54.4°C	57.0°C	59.7°C	62.3°C	65°C	67.6°C	69.9°C	72.0°C
Expected fragment	Strong	Strong	Strong	Strong	Strong	Strong	Strong	Strong	No	No
Primer dimer	No	No	No	No	No	No	No	No	No	No
Additional fragments	No	No	No	No	No	No	No	No	No	No

1.2.2 detection limit and fluorescence output signal

Standard solutions with 10^6 , 10^5 , 10^4 , 10^3 , 10^2 , 10 and 0 target copies per 2 µl were analyzed to determine the detection limit at optimal primer/probe concentrations. Fluorescent output signals were compared with the background to have at least a 100 fold increase in fluorescence signal. Reaction condition were adjusted if the fluorescence signal was too low in contrast to the background noise.

Results:

The detection limits (low and high) for qualitative detection was determined between 10 and $>10^6$ target copies per reaction. The detection limits (low and high) for quantitative detection was determined between 10 and $>10^6$ target copies per reaction. The fluorescence output signal was at least 100 (5 for positive sample, 0,05 for a negative sample) times stronger than the background signal. (fig. 4, table 9)

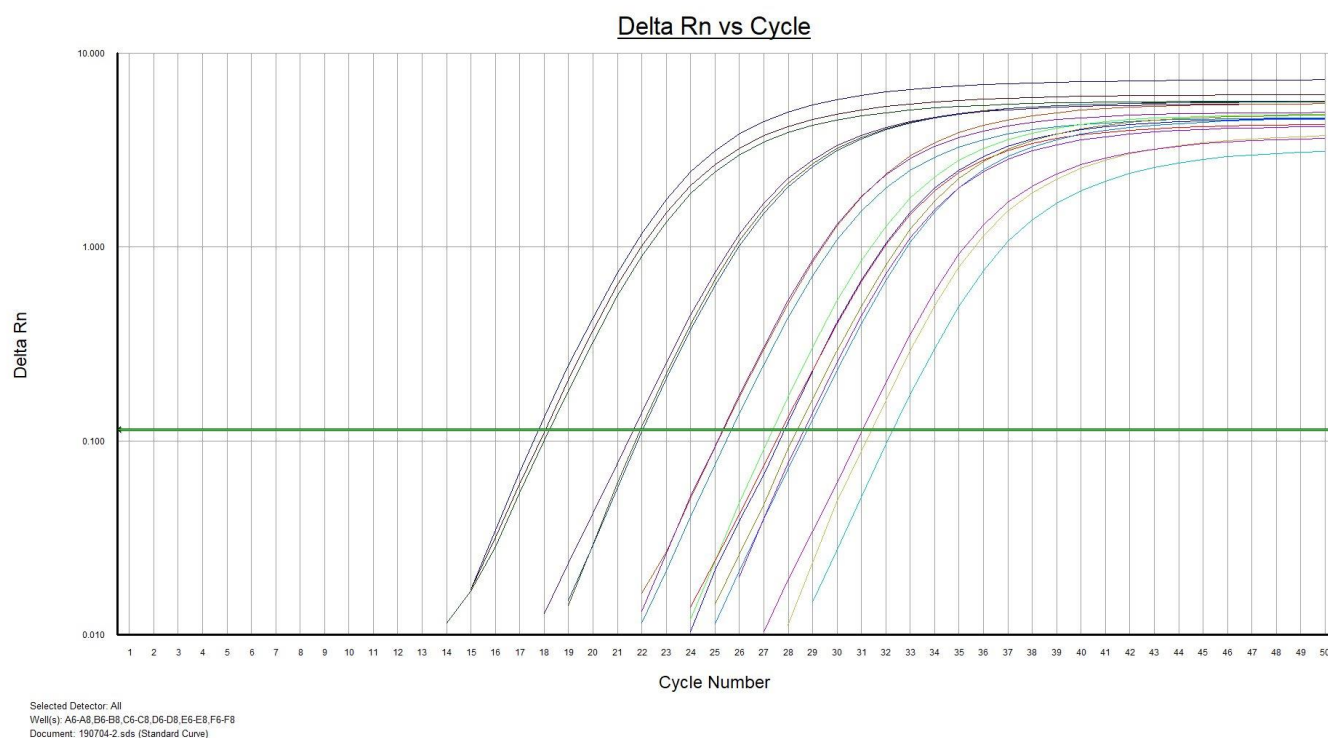


Figure. 4: Obtained fluorescent signal at optimal primer/probe concentration at a annealing temperature of 66°C.

Table 9: CT values obtained at optimal primer/probe concentration.

target DNA ¹ copy	Target detected	CT value	Standard deviation
0	No	-	-
10	Yes	31.5	0.6
10 ²	Yes	28.6	0.2
10 ³	Yes	27.6	0.3
10 ⁴	Yes	25.4	0.2
10 ⁵	Yes	21.9	0.1
10 ⁶	Yes	18.0	0.2

¹ Estimated by gel electrophoresis

² Not determined as very low amounts of DNA cannot reliable quantitatively detected by the qPCR technique

1.2.3 Efficiency

Based on the slope of the standard curve the efficiency of the primer/probe set was determined.

Results:

The efficiency of the test was above 90%. Which means that the efficiency of the primer/probe mixture can be regarded optimal (Fig. 5, table 10).

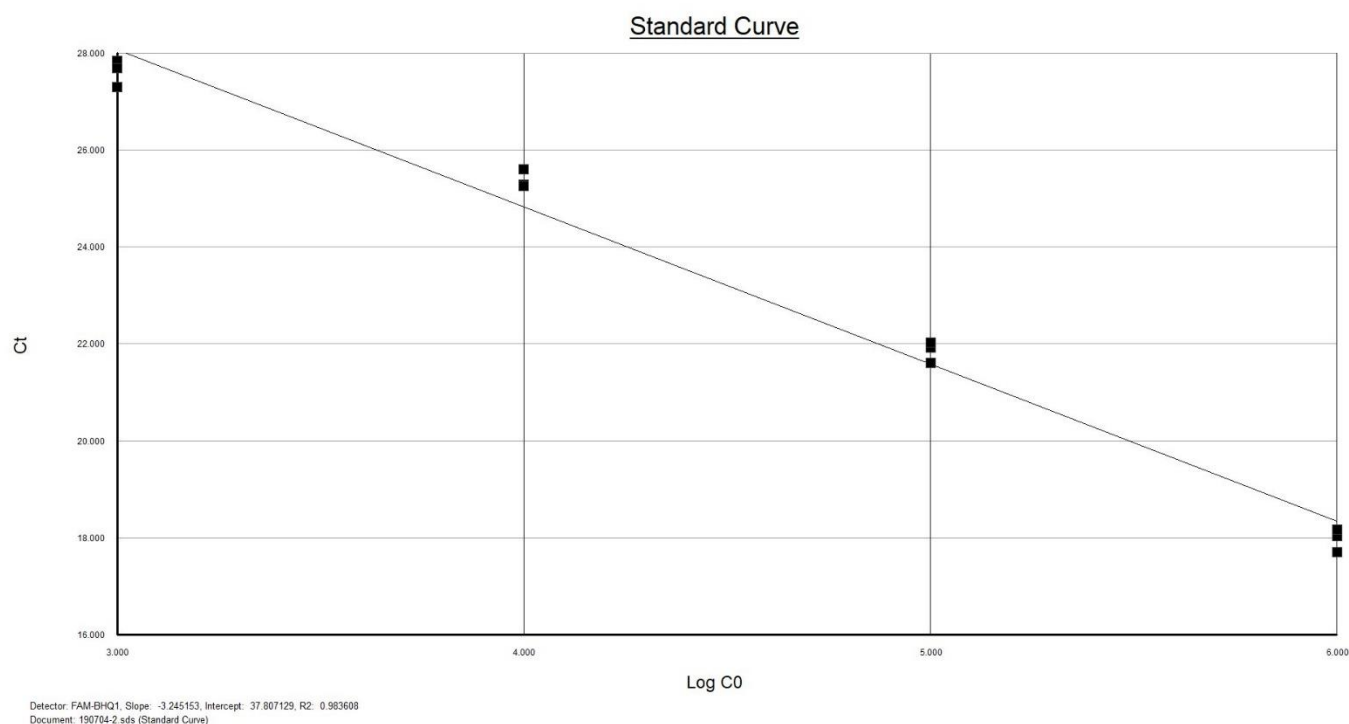


Fig. 5: Standard curve of SYL106 based on 10^3 , 10^4 , 10^5 and 10^6 DNA target copies

Table 10: Values obtained from the standard curve

Slope	-3.25
Efficiency	103.1%
R ²	0.98

1.2.4 Influence of inhibiting factors present in environmental samples and repeatability

Performance of the test was tested on the influence of inhibiting factors present in three different kinds of environmental water samples (sandy, clayey or peaty bottoms) in three fold spiked with 1000 target DNA copies. Standard deviations, difference to spike and the standard error of mean were calculated to determine robustness, repeatability and measurement uncertainty.

Results:

No fluorescent output signal was detected in the environmental samples without added target organism DNA (spike). Spiked samples and the spike only analyses gave in all replicates a positive signal. (see table 11). The difference between environmental samples and the spike only sample was less than 3%. Influence of chemical and biological factors present in environmental samples was not detected. The standard error of mean was 0.04 within these samples with an average of 27.4

Sample	CT value	Standard deviation	Difference to spike
Sandy	-	-	-
Clayey	-	-	-
Peaty	-	-	-
Sandy + spike	27.2	0.1	1.0%
Clayey + spike	26.8	0.3	2.5%
Peaty + spike	28.0	0.5	- 1.7 %
Spike only	27.5	0.1	-

Table 11: CT values obtained with target organisms free environmental samples spiked with 1000 target copies.

1.2.5 Detection conformation in environmental samples

Conformation of detection with the test was performed on samples from locations where the presence of *Thaumetopoea processionea* was suspected. Samples were taken using SYL001 - Environmental sampling kit and eDNA was isolated using SYL002 -Environmental DNA isolation kit.

Results:

The kit SYL110 – *Thaumetopoea processionea* detection kit was able to detect *Thaumetopoea processionea* in environmental samples from different locations in the Netherlands. On average, a positive sample gave 1 to 10 molecules *Thaumetopoea processionea* DNA when 100 ml water was filtrated.

1.2.6 Sequence conformation of specificity.

PCR products obtained from environmental samples were sequenced for conformation of identity of the formed product. If any product was formed with target organism free environmental samples, than these products were also be sequenced.

Results:

Target organism free environmental samples did not give any PCR product. PCR products obtained from environmental samples were sequenced in triplo via the Sanger sequencing method. The obtained sequences were identical to each other and Blast[®] hits confirmed identity of the target organism.

1.3 Summary of validation

1.3.1 Robustness

“Influence of temperature variations and inhibiting factors present in environmental samples on the performance and specificity of the primer set”

- Primers specific at temperature range: 50.0°C and 67.6°C (section 1.2.1, section 1.2.5, fig. 3, table 7)
- Influence of chemical and biological factors present in environmental samples on the performance of the test were not found. (section 1.4.2, table 9)
- Fluorescent output signals of positive samples is at least 100 fold stronger than the background

1.3.2 Detection limit

“Lowest limits in which the analysis can be reliably applied”

Limit of detection (LDqPCR) for this kit was determined on 1 copy per reaction. Limit of quantification (LQqPCR) was also determined on 10 copies per reaction. (section 1.2.2, table 8)

1.3.4 Efficiency

“The comparison of what is actually produced with what can be achieved with the same consumption of resources”

The efficiency of the primer set is 103.1 %, this means that the primer/probe mixture can be regarded as optimal. (section 1.2.3, table 9)

1.3.5 Repeatability

“The degree of similarity between the results of measurements of the same measured quantity that were performed under different measurement conditions”

There was no differences between different kinds of environmental water samples (sandy, clayey or peaty bottoms) spiked with 1000 target DNA copies. (section 4.2.4, table 9)

1.3.6 Correctness

“The ability of the method to do what it 'says' to do”

- The test was able to detect *Thaumetopoea processionea* DNA in environmental samples from locations where the presence of *Thaumetopoea processionea* was suspected. (section 1.2.6)
- The method did not give any other combined BLAST hit than the target organism *Thaumetopoea processionea*
- The method was able to detect all spiked target DNA in target organism free environmental samples (section 1.2.4, table 10)
- The method did not give any signal in target organism free environmental samples (section 1.2.4, table 11)
- The standard error of the mean based on the measured CT values from the spiked experiments (1000 target copies) was 0.04 on an average of 27.4.